

Operator: Validation Manager  
 Process: Validation  
 Session Start: 22-11-2013 09:31:31  
 Session Stop: 22-11-2013 09:31:37  
 Session Name: Retort Validation  
 Session Text:

Vessel: Retort  
 Product: Food  
 Time Zone: UTC offset 01:00:00




## Unit Configuration

Name: Retort Sterilization  
 Description:  
 Type: Retort

### Sensor Setup

Position:	Sensor S/N:	Label:	Position Name:	Position Description:	Sensor Alias:	Sensor group:	Sample Rate:
1	15392	1	Upper B1				00:00:01
2	15396	2	Medium B1				00:00:01
3	15338	3	Center B1				00:00:01
4	15395	4	Buttom B1				00:00:01
5	15390	5	Upper B2				00:00:01
6	15333	6	Medium B2				00:00:01
7	15337	7	Center B2				00:00:01
8	15393	8	Buttom B2				00:00:01
9	15336	9	Upper B3				00:00:01
10	15335	10	Medium B3				00:00:01
11	13826	11	Center B3				00:00:01
12	31726	12	Buttom B3				00:00:01
13	20962	13	Upper B4				00:00:01
14	15387	14	Medium B4				00:00:01
15	13832	15	Center B4				00:00:01
16	22085	16	Buttom B4				00:00:01

### Image Set 1

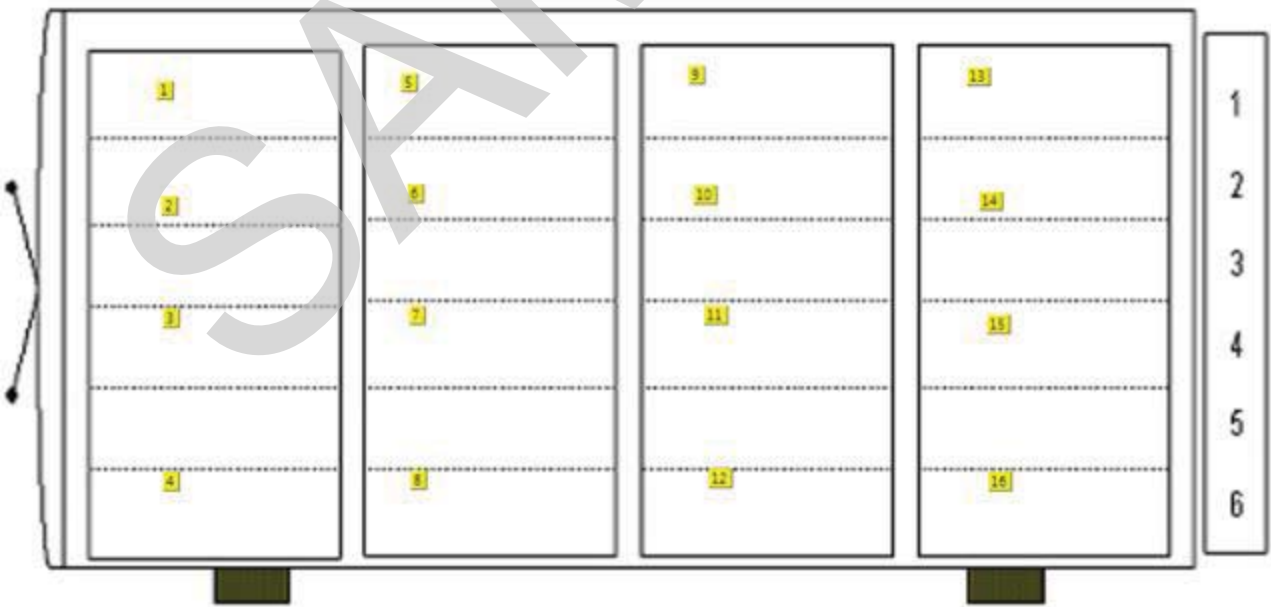

Operator: Validation Manager  
Process: Validation  
Session Start: 22-11-2013 09:31:31  
Session Stop: 22-11-2013 09:31:37  
Session Name: Retort Validation  
Session Text:

Vessel: Retort  
Product: Food  
Time Zone: UTC offset 01:00:00



## Image Set 1

